




KIMTECH PURE* A5 Sterile Apparel



DATA PACK



DATA PACK - KIMTECH PURE* A5 Sterile Cleanroom Apparel Contents

Description	Page Number
Product Information:	
A5 Sterile Cleanroom Coveralls	3
A5 Sterile Cleanroom Integrated Hood & Mask	4
A5 Sterile Cleanroom Boot Covers	5
A5 Sterile Cleanroom Sleeves	6
A5 Sterile Cleanroom Apparel Technical Performance Data	7
Gowning Posters:	
A5 Sterile Cleanroom Coveralls	8
A5 Sterile Cleanroom Integrated Hood & Mask	9
A5 Sterile Cleanroom Boot Covers	10
Label Designs:	
A5 Sterile Cleanroom Apparel Label design – Coveralls & Sleeves	11
A5 Sterile Cleanroom Apparel Label design – Hood and Integrated Hood & Mask	12
A5 Sterile Cleanroom Apparel Label design – Boot Covers	13
Certificates and Sterile Dose Validation	
A5 Sterile Cleanroom Apparel Certificate of Conformance (Example)	14
A5 Sterile Cleanroom Apparel Certificate of Irradiation (Example)	15
Sterile Dose Validation A5 Sterile Cleanroom Coveralls, Hoods and Boot Covers	16-36
Sterile Dose Validation A5 Sterile Cleanroom Integrated Hood & Mask	37-42
Sterile Dose Validation A5 Sterile Cleanroom Sleeves	43-48



CLEAN-DON*, the Revolution in Aseptic Gowning.

KIMTECH PURE* A5 Sterile Cleanroom Coveralls.

The KIMTECH PURE* A5 Sterile Cleanroom Coveralls simplify aseptic gowning to save time and reduce the risk of contamination.



CLEAN-DON* blue line on the inside indicates correct place to grasp for aseptic gowning.



Telescope fold and snaps prevent legs and arms falling to the floor during gowning.



Vacuum Packed and double bagged for added sterility assurance. Reduces space so more products fit into gowning area storage.



PERSONAL & PROCESS PROTECTION:

- Suitable for EU GMP ISO 5 Grade A cleanrooms
- Gamma Irradiated, Sterility Assurance Level 10⁻⁶
- Low Lint fabric, Helmke Drum test Category I
- Bacterial Filtration Efficiency 96%
- Manufactured and Packed in ISO 5 cleanroom
- Vacuum packed for sterility assurance, saves space
- Certified PPE Cat III directive 89/686/EEC
- Type 6 limited chemical splash protection
- Type 5 particle protection
- Breathable barrier combines comfort and protection

DESIGN FEATURES:

- Unhooded coverall available in size S to 4XL
- Blue Indicator line to avoid touching outside
- Presented unzipped with inside-out fold
- Arms and legs telescope folded with snaps
- Waist and back panel elastics
- Elastic cuffs and thumb loops
- High strength, bound and triple stitched seams
- High performance SMS breathable barrier
- Individually vacuum packed and double bagged.
- 25 items per double case liner.

Applications:

EU GMP
ISO 5 Grade A

Aseptic
Processing


Parenteral
Drug
Manufacturing

Biotechnology

Pharmaceutical
Compounding

Ophthalmic
product
manufacturing

Aseptic Hood
work



CLEAN-DON*, the Revolution in Aseptic Gowning.

KIMTECH PURE* A5 Sterile Integrated Hood & Mask.

The KIMTECH PURE* A5 Sterile Integrated Hood & Mask simplifies aseptic gowning to save time and reduce the risk of contamination.



CLEAN-DON* blue line on the inside indicates correct place to grasp for aseptic gowning. Saves time and reduces contamination risk.



No gaps between hood and mask ensures exhaled air is filtered.
Elastics provide a comfortable, secure and universal fit.



Vacuum packed for added sterility assurance. Reduces space so more products fit into gowning area storage.



STERILE R

PERSONAL & PROCESS PROTECTION:

- Suitable for EU GMP ISO 5 Grade A cleanrooms
- Gamma Irradiated, Sterility Assurance Level 10⁻⁶
- Low Lint fabric, Helmke Drum test Category I
- Bacterial Filtration Efficiency 96%
- Manufactured and Packed in ISO 5 cleanroom
- Vacuum packed for sterility assurance, saves space
- Certified PPE Cat III directive 89/686/EEC
- Type 6 Pb limited chemical splash protection
- Breathable barrier combines comfort and protection

DESIGN FEATURES:

- Integrated hood and mask
- Stretch fit elastics for universal size
- Blue Indicator line to avoid touching outside
- Pull down ties on back to assist gowning
- Presented inside-out fold to avoid contamination
- High strength, bound and triple stitched seams
- High performance SMS with cloth-like feel
- Individually vacuum packed
- 25 items per double-bag, 3 double bags per case

Applications:

EU GMP
ISO 5 Grade A

Aseptic
Processing

Parenteral
Drug
Manufacturing


Biotechnology

Pharmaceutical
Compounding

Ophthalmic
product
manufacturing

Aseptic Hood
work





CLEAN-DON*, the Revolution in Aseptic Gowning.

KIMTECH PURE* A5 Sterile Cleanroom Boot Covers.

The KIMTECH PURE* A5 Sterile Boot Covers improves worker safety and comfort, while reducing the risk of contamination.



New Version Ideal for wet applications.
Wrap-around Vinyl foot is seamed above the floor line to reduce risk of liquid penetration and trip hazards.
Standard vinyl sole also available.



3 sizes for better safety and comfort.
Better fit and comfort to improve worker safety by reducing risk of trip hazards.



Vacuum packed for added sterility assurance. Reduces space so more products fit into gowning area storage.



PROCESS PROTECTION:

- Suitable for EU GMP ISO 5 Grade A cleanrooms
- Gamma Irradiated, Sterility Assurance Level 10⁻⁶
- Low Lint fabric, Helmke Drum test Category I
- Bacterial Filtration Efficiency 96%
- Manufactured and Packed in ISO 5 cleanroom
- Vacuum packed for sterility assurance, saves space
- CE 89/686/EEC Category I PPE – simple design
- Breathable barrier combines comfort and protection

DESIGN FEATURES:

- New Vinyl foot version available in 3 sizes.
- Standard Vinyl sole version available in 3 sizes.
- Elastic opening presented inside-out folded.
- Two extra-long ties.
- SMS material cloth-like feel keeps gloves in place
- High strength, bound and triple stitched seams
- Individually vacuum packed pairs
- 25 pairs per double-bag, 4 double bags per case

Applications:

EU GMP
ISO 5 Grade A

Aseptic
Processing

Parenteral
Drug
Manufacturing

Biotechnology

Pharmaceutical
Compounding

Ophthalmic
product
manufacturing

Aseptic Hood
work





CLEAN-DON*, the Revolution in Aseptic Gowning.

KIMTECH PURE* A5 Sterile Cleanroom Sleeves.

The KIMTECH PURE* A5 Sterile Cleanroom Sleeves simplify aseptic gowning to save time and reduce the risk of contamination.



CLEAN-DON* blue line on the inside indicates correct place to grasp for aseptic gowning. Thumb-loops and material's cloth-like feel keep sleeves and gloves in place.



Telescoped fold makes aseptic gowning easier, preventing contact with the outside surface to reduce contamination risk.



Vacuum packed for added sterility assurance. Reduces space so more products fit into gowning area storage.



PROCESS PROTECTION:

- Suitable for EU GMP ISO 5 Grade A cleanrooms
- Gamma Irradiated, Sterility Assurance Level 10⁻⁶
- Low Lint fabric, Helmke Drum test Category I
- Bacterial Filtration Efficiency 96%
- Manufactured and Packed in ISO 5 cleanroom
- Vacuum packed for sterility assurance, saves space
- CE 89/686/EEC Category I PPE – simple design
- Breathable barrier combines comfort and protection

DESIGN FEATURES:

- 45cm long sleeve protectors, pair packed.
- Blue Indicator line to avoid touching outside
- Telescope inside-out fold for easy gowning
- Elastic cuffs and thumb loops
- SMS material cloth-like feel keeps gloves in place
- High strength, bound and triple stitched seams
- Individually vacuum packed pairs
- 25 pairs per double-bag, 4 double bags per case

Applications:

EU GMP
ISO 5 Grade A

Aseptic
Processing

Parenteral
Drug
Manufacturing

Biotechnology

Pharmaceutical
Compounding

Ophthalmic
product
manufacturing

Aseptic Hood
work





KIMTECH PURE* A5 Sterile Cleanroom Apparel Technical Data

Quality Standards

- Suitable for ISO 5 Grade A Sterile Cleanrooms
- Manufactured in ISO9001 and ISO13485 certified facility
- Sterility Assurance Level 10⁻⁶ and Helmke Drum test Category I
- Sterilization in accordance with EN556-1, EN ISO11737-1,-2, EN ISO 11140-1

Fabric Tests		Test Method	Result
Particle shedding test (Helmke Drum)		IEST-RP-CC003.3	Category I
Bacterial Filtration Efficiency (3.0 µm) - SMS material in A5 fabric		ASTM F2100	96%
Bacterial Filtration Efficiency (3.0 µm) - Mask in iHAM		ASTM F2100	94%
Particle filtration Efficiency (0.5 µm) - SMS material A5 fabric		ASTM F2299	94%
Particle Filtration Efficiency (0.5 µm) - Mask in iHAM		ASTM F2299	93%
Abrasion resistance		EN 530 Method 2	Class 3 of 3
Flex cracking resistance		ISO 7854 Method B	Class 5 of 6
Trapezoidal tear resistance		ISO 9073-4	Class 2 of 3
Puncture resistance		EN 863	Class 1 of 3
Tensile strength		EN ISO 13934-1	Class 1 of 3
Resistance to ignition		EN 13274-4 Method 3	Pass
Seam strength		EN ISO 13935-2	Class 3 of 3

EN ISO 6350:2005 – Resistance of penetration by liquids/chemicals.	CAS number	Penetration Class	Penetration %	Repellency Class	Repellency %
1-butanol 100%	71-36-3	3	<1%	1	>80%
Ethanol 70%	64-17-5	3	<1%	2	>90%
Ethylene glycol 100%	107-21-1	3	<1%	2	>90%
Incidin Plus 100%	N/A	3	<1%	2	>90%
Isopropyl Alcohol 70%	67-63-0	2	<5%	1	>80%
Sekusept plus	N.A	3	<1%	2	>90%
Sodium Hydroxide 10%	1310-73-2	3	<1%	3	>95%
Sulphuric Acid 30%	7664-93-9	3	<1%	2	>90%

KIMTECH PURE* A5 Sterile Cleanroom Apparel

Description	Code.	Description	Code.
Coveralls, 25 per Case	88800 (S), 88801 (M), 88802 (L), 88803 (XL), 88804 (2XL), 88805 (3XL), 88806 (4XL)	Integrated Hood & Mask, 75 per Case	36072
Boots Vinyl Foot, 100 pairs per Case	12922 (S), 88808 (Universal), 12920 (XL)	Hood with Ties, 100 per Case	25797 / 88807
Boots Vinyl Sole, 100 pairs per Case	31683 (S), 31696 (Universal), 31697 (XL)	Sterile Sleeves, 100 pairs per Case	36077

Gowning Procedure

BEFORE GOWNING

Step 1: (Pre-Entry) Don Hair Net and Shoe Covers after removing all jewelry and cosmetics.

Step 2: (Gowning) Wash hands and gown first pair of sterile gloves. Sanitize gloves after gowning each article if required.

Step 3: Apply mask and hood assuring a snug fit.

Step 4: Open vacuumed-packed apparel.
Tear at notched edge.



Step 5: Grasp the blue line.
Located on the inside middle back.



Step 6: Gently unfold coverall utilizing blue indicator line. Arms and legs are pre-drawn and snapped in place. Garment is already folded inside-out and unzipped.

BEGIN GOWNING

Snaps allow gathered-up arms and legs to expand during gowning



Step 7: Hold garment at waist



Step 8: Put one leg in and point toe through opening until snap releases



Step 9: Do the same with the other leg



Step 10: Insert one arm and extend until snap releases



Step 11: Do the same with the other arm



Step 12: Slip thumbs through thumb loops



Final Step: Cross legs and zip up coverall



After A5 Sterile Cleanroom Apparel is Gowned:

Add boot covers



Complete gowning by adding goggles and a second pair of sterile gloves.

KIMTECH PURE* A5 Integrated Hood and Mask Donning Technique



Step 1

Select your integrated hood and mask; inspect package for vacuum seal; tear along notches toward the product to open



Step 2

Pull out integrated hood and unfold to locate the blue signal indicator line



Step 3

Center your chin just above the blue line then roll over your forehead.



Step 4

Grab ties with both hands then extend arms out in a circular motion to position under armpits.



Step 5

Pull ties across chest and secure as needed



Step 6

Gently adjust front flap to comfortable position; pinch mask wire over bridge of nose to ensure proper fit.



KIMTECH PURE* A5 Sterile Boot Cover with Grasp Ties Donning Technique



Step 1

Select your boot cover size; inspect package for vacuum seal; tear along notches toward the product to open; flex package to separate boot covers



Step 2

Pull out one boot cover by the cuff



Step 3

Grasp ties with one hand and make sure they don't touch the floor



Step 4

Open up boot cover; point toe towards opening and pull up over calf while holding the ties



Step 5

Hold up foot or rest on bench. Grasp ties at front of boot cover and wrap over cusp of shoe/boot; then wrap ties behind ankle and tie in front.



Step 6

Place donned boot on the clean side



Step 7

Pull the remaining boot cover out of package by the cuff and repeat Steps 3, 4 and 5. Proceed with final gowning steps



Exceptional
Workplaces*

KIMTECH
PURE* BRAND



KIMTECH PURE* A5 Sterile Cleanroom Apparel
Label Design

A5 Sterile Cleanroom Coveralls
88800 (S), 88801 (M), 88802 (L), 88803 (XL)
88804 (2XL), 88806 (3XL), 88806 (4XL)

A5 Sterile Cleanroom Sleeves
36072 – one size fits all

Case Label

88803 10

25 White Coveralls
XL
25 Combinaisons blanches
TG
25 Overoles blancos
XG
25 Weiße Overalls
XL
Белые комбинезоны: 25 штук
XL

LOT # 1234567890

1234-56

Made in China
Fabriqué en Chine
Fabricado en China
Hergestellt in China
Сделано в Китае

1 00 36000 88803 1

088902_01

36077 00

100 Pair
Sleeves with CLEAN-DON® Technology
One size fits all
100 paires
Manches avec technologie CLEAN-DON®
Taille universelle
100 pares
Mangas con tecnologia CLEAN-DON®
Talla única
100 Paar
Ärmel mit CLEAN-DON® Technologie
Eine Größe passt allen
100 пар
Рукава по технологии CLEAN-DON®
Один размер для всех

LOT #

Made in China
Fabriqué en Chine
Fabricado en China
Hergestellt in China
Сделано в Китае

1 00 36000 36077 3

Item Label

Kimberly-Clark
PROFESSIONAL®

KIMTECH
PURE* BRAND

A5

Cleanroom Apparel
 Vêtements pour salle blanche
 Vestimenta para sala limpia
 Reinraumkleidung
 Одежда для чистых комнат

1

Made from 100% polyolefin
Fabriquées en polyoléfine
Hecho 100% de poliolefinas
Hergestellt aus 100% Polyolefin
Изготовлено из 100% полиолефина

REF 88803

XL

1234-56

1234567890

CE 0120

© / * Trademarks of Kimberly-Clark Worldwide, Inc.
Marques déposées de Kimberly-Clark Worldwide, Inc.
© 2007 KCWW
Made in China / Fabriqué en Chine
www.kcpprofessional.com

082248_028
20-20-4520-02

Kimberly-Clark
PROFESSIONAL®

KIMTECH
PURE* BRAND

A5

Cleanroom Sterile Sleeves
with CLEAN-DON® Technology
 Salle blanche stérile - Manches avec technologie CLEAN-DON®
 Estériles para sala limpia - Mangas con tecnologia CLEAN-DON®
 Reinraum-steril - Ärmel mit CLEAN-DON® Technologie
 Стерильные продукты для чистых помещений - Рукава по технологии CLEAN-DON®

REF 36077

1 Pair/Sleeves with CLEAN-DON® Technology
Paire/manches avec technologie CLEAN-DON®
Par / Mangas con tecnologia CLEAN-DON®
Paar/Ärmel mit CLEAN-DON® Technologie
Пара/Рукава по технологии CLEAN-DON®

One size fits all
Taille universelle
Talla única
Eine Größe passt allen
Один размер для всех

CE

Made from 100% polyolefin
Fabriquées en polyoléfine
Hecho 100% de poliolefinas
Hergestellt aus 100% Polyolefin
Изготовлено из 100% полиолефина

© / * Trademarks of Kimberly-Clark Worldwide, Inc.
Marques déposées de Kimberly-Clark Worldwide, Inc.
© 2007 KCWW
Made in China / Fabriqué en Chine
www.kcpprofessional.com

20-20-4520-00



KIMTECH PURE* A5 Sterile Cleanroom Apparel
Label Design

A5 Sterile Cleanroom Hoods with ties
EU 88807(01) / US 25797(00)

A5 Sterile Integrated Hood & Mask
36072 – one size fits all

Case Label

US 25797 00
EU 88807 01

100 Sterile Hoods with Ties
One size fits all
100 capuchons stériles avec attaches
Taille unique
100 capuchas estériles, con cintas
Una sola talla
100 Sterile Hauben mit Bändern
Eine Größe passt allen
100 стерильных напюшонов с завязками
Безразмерный

LOT #

STERILE R

Made in China
Fabriqué en Chine
Fabricado en China
Herstellt in China
Сделано в Китае

1 00 36000 25797 4

36072 00

75 Integrated Hood and Mask with CLEAN-DON® Technology
One size fits all
75 Capuche et masque intégrés avec technologie CLEAN-DON®
Taille universelle
75 Capuchón y mascarilla integrados con tecnología CLEAN-DON®
Talla única
75 Integrierte Haube und Maske mit CLEAN-DON® Technologie
Eine Größe passt allen
75 Интегрированный капюшон с маской по технологии CLEAN-DON®
Один размер для всех

LOT #

STERILE R

Made in China
Fabriqué en Chine
Fabricado en China
Herstellt in China
Сделано в Китае

1 00 36000 36072 8

Item Label

Kimberly-Clark
PROFESSIONAL®

KIMTECH
PURE* BRAND

A5

④ Cleanroom Apparel
④ Vêtements pour salle blanche
④ Vestimenta para sala limpia
④ Reinraumkleidung
④ Одежда для чистых комнат

1 Sterile Hood with Ties / One size fits all
1 Capuchon stériles avec attaches / Taille unique
1 Capuchon estériles, con cintas / Una Sola Talla
1 Sterile Haube mit Bändern / Eine Größe passt allen
1 стерильных напюшонов с завязками / Безразмерный

LOT

STERILE R

PB(6)

CE 0120
EN13054: 2005

AB37

Made from 100% polyolefin
Fabriqué en polyoléfine
Hecho 100% de poliolefina
Hergestellt aus 100% Polyolefin
Изготовлено из 100%-ного полиолефина

© / * Trademarks of Kimberly-Clark Worldwide, Inc.
Marques déposées de Kimberly-Clark Worldwide, Inc.
© 2007 KCVW.
Made in China / Fabriqué en Chine
www.kcprofessional.com

03551_578
20-30-01-001

Kimberly-Clark
PROFESSIONAL®

KIMTECH
PURE* BRAND

A5

④ Cleanroom Sterile Integrated Hood and Mask with CLEAN-DON® Technology
④ Salle blanche stérile - Capuche et masque intégrés avec technologie CLEAN-DON®
④ Estériles para sala limpia - Capuchón y mascarilla integrados con tecnología CLEAN-DON®
④ Reinraum-steril - Integrierte Haube und Maske mit CLEAN-DON® Technologie
④ Стерильные продукты для чистых помещений - Интегрированный капюшон с маской по технологии CLEAN-DON®

1 Integrated Hood and Mask with CLEAN-DON® Technology
One size fits all
Taille universelle
Talla única
Eine Größe passt allen
Один размер для всех

LOT

STERILE R

PB(6)

CE 0120
EN13054: 2005

Mommen material is 100% polyolefin; face mask includes malleable wire component.
Le matériau non tissé est fabriqué en 100 % polyoléfine; le masque facial comprend une barrette malléable.
La tela no tejida es de 100% poliolefina; la mascarilla incluye un alambre maleable.
Das nichtgewebte Material ist 100% Polyolefin; die Gesichtsmaske enthält eine biegbare Drahtkomponente.
Нечалый материал, изготовленный из 100% полиолефина; маск содержит гибкие проволочные компоненты.

© / * Trademarks of Kimberly-Clark Worldwide, Inc.
Marques déposées de Kimberly-Clark Worldwide, Inc.
© 2007 KCVW.
Made in China / Fabriqué en Chine
www.kcprofessional.com

20-30-01-001

Please note:

From June 2013 production, 88807(01) will be dual coded to 25797 (US) / 88807 (EU).

This product is identical in design and specification.

Our European business will continue to refer to this product as 88807 in all price lists, literature and ordering systems.



KIMTECH PURE* A5 Sterile Cleanroom Apparel
Label Design

A5 Sterile Boot Covers with Vinyl Sole
12922 (S), 88808 (Universal), 12920 (XL)

A5 Sterile Boot Covers with Vinyl Foot
31683 (S), 31696 (Universal), 31697 (XL)

Case Label

88808 10

Boots
100 Pair
One size fits all
Bottes
100 Paire
Taille unique
Botas
100 Par
Una sola talla
Stiefel
100 Paare
Eine Größe passt allen
Ботинки
100 пар
Безразмерный

LOT # 1234567890

1234-56

STERILE R

Made in China
Fabriqué en Chine
Fabricado en China
Hergestellt in China
Сделано в Китае

1 00 36000 88808 6

083078_003

31683 00

Boots
100 Pair • Small/Medium
Bottes
100 Paire • Petites/Moyennes
Botas
100 Par • Pequeñas/Medianas
Stiefel
100 Paare • Klein/Mittel
Ботинки
100 пар • Маленький размер/Средний размер

LOT #

STERILE R

Made in China
Fabriqué en Chine
Fabricado en China
Hergestellt in China
Сделано в Китае

1 00 36000 31683 1

Item Label

Kimberly-Clark
PROFESSIONAL*

KIMTECH
PURE* BRAND

A5

EN Cleanroom Apparel
FR Vêtements pour salle blanche
ES Vestimenta para sala limpia
DE Reinraumkleidung
RU Одежда для чистых комнат

Made from 100% polyolefin
Fabriquées en polyoléfine
Hecho 100% de poliolefina.
Hergestellt aus 100 % Polyolefin
Изготовлено из 100%-ного полиолефина

© / * Trademarks of Kimberly-Clark Worldwide, Inc.
Marques déposées de Kimberly-Clark Worldwide, Inc.
© 2007 KCWW.
Made in China / Fabriqué en Chine
www.kcprofessional.com

AB37

052828_264
20-30-438-0-00

REF 88808

1 Pair/Boots
Paire/Bottes
Par/Botas
Paar/Stiefel
Пара/Ботинки

One size fits all
Taille unique
Una Sola Talla
Eine Größe passt allen
Безразмерный

1234-56

LOT 1234567890

STERILE R

REF 31683

1 Pair/Boots
Paire/Bottes
Par/Botas
Paar/Stiefel
Пара/Ботинки

Small/Medium
Petites/Moyennes
Pequeñas/Medianas
Klein/Mittel
Маленький размер/
Средний размер

LOT

STERILE R



Certificate of Conformance KIMTECH PURE* A5 Cleanroom Sterile Apparel

Product: **KIMTECH PURE* A5 Cleanroom Sterile Apparel**

Code	Description	Size	Packaging
88800	Coverall	S	25/case
88801	Coverall	M	25/case
88802	Coverall	L	25/case
88803	Coverall	XL	25/case
88804	Coverall	2XL	25/case
88805	Coverall	3XL	25/case
88806	Coverall	4XL	25/case
12917	Coverall	5XL	25/case
12914	Coverall	6XL	25/case
88807	Hood, no ties	One-Size	100/case
25797	Hood, with ties	One-Size	100/case
88808	Universal Boots	One-Size	100 pr/case
12922	Boots	S/M	100 pr/case
12920	Boots	XL/2XL	100 pr/case
31683	Boots, with edge vinyl	S/M	100 pr/case
31696	Boots, with edge vinyl	One-Size	100 pr/case
31697	Boots, with edge vinyl	XL/2XL	100 pr case

Lot number: XN213701X

This document certifies that the lots listed above conform to Kimberly-Clark's internal specifications for product quality. Kimberly-Clark uses a system of in-process and lot inspections to assure conformance to specifications.


Characteristic	Specification Target
Particle Count (Helmke Drum, IEST-RP-CC003.3)	Category I ¹
Sterility Assurance Level (ANSI/AAMI/ISO 11137)	10 ⁻⁶

A Certificate of Irradiation is also available to assure that the product has received the specified radiation dosage.

Verified by:  Date: May 29, 2012

© Registered Trademark and * Trademark of Kimberly-Clark Worldwide, Inc. © 2006 KCWW. All Rights Reserved.

¹Product is tested prior to sterilization
Customer Service: 800-255-6401



辐照证明书

CERTIFICATE OF IRRADIATION



深圳市金鹏源辐照技术有限公司
 SHENZHEN JPY ION-TECH CO., LTD.
 地址 (Add): 深圳市罗湖区布心东盛路68号
 No.68 Dongsheng Rd., Buxin, Luohu, Shenzhen 518019 China
 电话 (TEL): +86(0)755 25177231, 25177137
 传真 (FAX): +86(0)755 25516854
 邮政编码 (P.C.): 518019
 http://www.jpym.com.cn

证书编号: GM2012071502
 Certificate No.:
 分合同编号: GM12070127
 Sub-contract:

R/SZJPY(B)-7515 AC/01

客户名称 Customer: Kimberly-Clark Professional				
产品名称 Article description	包装规格(厘米) Carton Size(cm)	产品批号 Article Lot No.	数量(箱) Carton Qty(cs)	毛重(公斤) G.W(kgs)
Universal Boots:88808	50*30*37	XN218101X	*180*	1620
Sleeve:36077	50*30*37	XN218801X	*62*	334.8
Coverall: 88802	50*30*37	XN213701X	*22*	158.4
Coverall: 88805	50*30*42	XN213701X	*75*	645
Universal Boots:88808	50*30*37	XN218801X	*40*	360
以下空白				
这批产品已经过伽玛射线辐照。 THE PRODUCTS HAVE BEEN IRRADIATED BY GAMMARAY.				
加工编号 Process Code No.		P1207153		
辐照结束的日期 Irradiation lot finish date		2012-07-15		
客户要求最低吸收剂量: Minimum specified dose:		最低剂量监测区吸收剂量: Minimum inspection area dose:		
32.5 kGy		34.0 kGy		
客户要求最高吸收剂量: Maximum specified dose:		最高剂量监测区吸收剂量: Maximum inspection area dose:		
50 kGy		44.6 kGy		
检验员: Inspector:		深圳市金鹏源辐照技术有限公司 光明分公司 SHENZHEN JPY ION-TECH CO., LTD. GUANGMING BRANCH		
审核: Approved:				
日期: Date:				
2012-7-15				



SteriPro.
Consulting

A Division of
Sterigenics International, Inc.

Protocol Number	Revision	Issue Date	Brief Description of Revision
797100277-P	0	April 12, 2010	
	1		
	2		

Protocol Title

**VD-Max32.5 Radiation Validation for KIMTECH PURE* A5
Cleanroom Sterile Apparel**

SteriPro Consultant: Zabrina Tumaitis

Sponsor Name and Address:
Kimberly-Clark
1400 Holcomb Bridge Road
Roswell, GA 30076

Sponsor Contact:
Theresa McCoy

Prepared By:

Zabrina Tumaitis
Consultant, SteriPro Consulting

Date

Reviewed By:

Julie Arinaga
Quality Assurance Manager, SteriPro Labs

Date

Approved By:

Niki Fidopiastis
Director, SteriPro Consulting

Date

Approved By:

Theresa McCoy

Theresa McCoy
Kimberly-Clark

April 14, 2010

Date

SteriPro will maintain copies of all Protocols, Final Reports, and supporting documentation for a retention period of five (5) years from the report issue date. After this period, SteriPro will contact the sponsor for disposition of these materials.

Confidential



Protocol Number	Revision	Issue Date	Brief Description of Revision
797100277-P	0	April 12, 2010	
	1		
	2		

Protocol Title VD-Max32.5 Radiation Validation for KIMTECH PURE* A5 Cleanroom Sterile Apparel	
SteriPro Consultant: Zabrina Tumaitis	
Sponsor Name and Address: Kimberly-Clark 1400 Holcomb Bridge Road Roswell, GA 30076	Sponsor Contact: Theresa McCoy

Prepared By: _____ Date _____
 Zabrina Tumaitis
 Consultant, SteriPro Consulting

Reviewed By: _____ Date _____
 Julie Arinaga
 Quality Assurance Manager, SteriPro Labs

Niki Fidopiastis

Digitally signed by Niki Fidopiastis
 DN: cn=Niki Fidopiastis, o=Director of Consulting,
 ou=SteriPro, email=nfidopiastis@sterigenics.com,
 c=US
 Date: 2010.04.14 07:34:02 -07'00'

Approved By: _____ Date _____
 Niki Fidopiastis
 Director, SteriPro Consulting

Approved By: _____ Date _____
 Theresa McCoy
 Kimberly-Clark

SteriPro will maintain copies of all Protocols, Final Reports, and supporting documentation for a retention period of five (5) years from the report issue date. After this period, SteriPro will contact the sponsor for disposition of these materials.

Confidential



SteriPro.
Consulting

A Division of
Sterigenics International, Inc.

Protocol Number	Revision	Issue Date	Brief Description of Revision
797100277-P	0	April 12, 2010	
	1		
	2		

Protocol Title

**VD-Max32.5 Radiation Validation for KIMTECH PURE* A5
Cleanroom Sterile Apparel**


SteriPro Consultant: Zabrina Tumaitis

Sponsor Name and Address:
Kimberly-Clark
1400 Holcomb Bridge Road
Roswell, GA 30076

Sponsor Contact:

Theresa McCoy

Prepared By:


Zabrina Tumaitis
Consultant, SteriPro Consulting

12 April 2010
Date

Reviewed By:


Julie Arinaga
Quality Assurance Manager, SteriPro Labs

4-13-10
Date

Approved By:

Niki Fidopiastis
Director, SteriPro Consulting

Date

Approved By:

Theresa McCoy
Kimberly-Clark

Date

SteriPro will maintain copies of all Protocols, Final Reports, and supporting documentation for a retention period of five (5) years from the report issue date. After this period, SteriPro will contact the sponsor for disposition of these materials.

Confidential



SteriPro.
Consulting
A Division of
Sterigenics International, Inc.

VD-Max32.5 Radiation Validation
Kimberly-Clark

Issued April 12, 2010
Protocol # 797100277-P Rev.0
Page 2 of 8

Terms and Conditions of Study

Any and all reports and letters issued by SteriPro Consulting or SteriPro Laboratories, divisions of Sterigenics U.S., LLC (collectively referred to as "Sterigenics") are for the sole and exclusive use of Sterigenics and the sponsor to whom they are addressed. Sterigenics strictly prohibits any other use or reproduction of any reports or portions thereof, quotations from any such reports or use of Sterigenics' name without Sterigenics' prior written consent. Sponsor acknowledges and shall be deemed to have agreed, upon its use of Sterigenics' services that the significance of any data is subject to the adequacy and representative character of the samples tendered for testing. Sterigenics warrants only that all tests are performed in accordance with established laboratory procedures and standards. Sterigenics makes no other warranties or representations of any kind, express or implied, including but not limited to anything regarding the adequacy of the samples tendered for testing for any specific use or application, such determination being the sole responsibility of the sponsor. Sponsor acknowledges and shall be deemed to have agreed, upon its use of Sterigenics' services, that Sterigenics' liability for any loss or damage resulting from Sterigenics' acts or omissions shall in no event exceed the cost of tests performed. In no event shall Sterigenics be liable for any special, indirect, incidental, consequential, punitive or other similar damages, including but not limited to damages arising from death, bodily injury, property damage (other than as set forth herein), loss of profits or revenue or loss of use of any samples or products.



SteriPro.
Consulting
A Division of
Sterigenics International, Inc.

VD-Max32.5 Radiation Validation
Kimberly-Clark

Issued April 12, 2010
Protocol # 797100277-P Rev.0
Page 3 of 8

Table of Contents

Title	Page
1. Scope	4
2. Objectives	4
3. Rationale	5
4. Terms and Definitions	5
5. Responsibilities	5
6. Product Specifications	5
7. Bioburden Study Method	6
8. Verification Study Method	6
9. Acceptance Criteria	7
10. Routine Sterilization	8
11. References	8



1. Scope

This study will be performed to establish a 32.5-kGy minimum dose and validate the effectiveness of Gamma Radiation sterilization of the KIMTECH PURE* A5 Cleanroom Sterile Apparel. Please refer to the Product Family Members Table below for all products included in this sterilization family. This protocol describes procedures for validation of radiation sterilization of medical products in accordance with AAMI TIR 33: *Sterilization of health care products – Radiation – Substantiation of a selected sterilization dose – Method VD-Max.*

Product Family Members
Description
Kimtech Pure* A5 Cleanroom Sterile Apparel - Coveralls - Size S
Kimtech Pure* A5 Cleanroom Sterile Apparel - Coveralls - Size M
Kimtech Pure* A5 Cleanroom Sterile Apparel - Coveralls - Size L
Kimtech Pure* A5 Cleanroom Sterile Apparel - Coveralls - Size XL
Kimtech Pure* A5 Cleanroom Sterile Apparel - Coveralls - Size 2XL
Kimtech Pure* A5 Cleanroom Sterile Apparel - Coveralls - Size 3XL
Kimtech Pure* A5 Cleanroom Sterile Apparel - Coveralls - Size 4XL
Kimtech Pure* A5 Cleanroom Sterile Apparel - Coveralls - Size 5XL
Kimtech Pure* A5 Cleanroom Sterile Apparel - Coveralls - Size 6XL
Kimtech Pure* A5 Cleanroom Sterile Apparel - Hoods - One size fits all
Kimtech Pure* A5 Cleanroom Sterile Apparel - Boots – Size S/M
Kimtech Pure* A5 Cleanroom Sterile Apparel - Boots – Size L
Kimtech Pure* A5 Cleanroom Sterile Apparel - Boots – XL/2XL

2. Objectives

- 2.1. Preliminary bioburden data has determined the Kimtech Pure* A5 Cleanroom Sterile Apparel - Coveralls - Size 6XL as the Dose Setting Device for this sterilization family.
- 2.2. The Dose Setting Device for the product family will be the test sample for this validation. Pre-sterilization bioburden level will be determined to establish the appropriate verification dose.
- 2.3. Recommendation for a routine minimum sterilization dose will be based on evaluation of microbial survivors following exposure of products to the verification dose. The minimum dose of 32.5 kGy will be designed to provide a Sterility Assurance Level (SAL) of 10^{-6} or not more than one non-sterile unit for each one million units sterilized at that dose level.
- 2.4. This study is intended to support release of products for which exposure to the minimum required dose can be demonstrated by the use of calibrated dosimeters and without post-exposure sterility testing of each lot.



3. Rationale

- 3.1. The VD-Max validation is utilized to determine the minimum effective processing dose for radiation sterilization. The validation is based on the concept that the product bioburden for the overall average or a single lot average (if greater than twice the overall average) bioburden will be less than 100,000 colony forming units.
- 3.2. The VD-Max procedure analyzes the number and resistance of the bioburden on the product. Three independent lots of product are tested for bioburden levels, and the bioburden recovery efficiency (percent recovery) is determined. The bioburden recovery efficiency and the sample item portion (percent of unit tested) are used to calculate the theoretical device bioburden on each test unit. The final bioburden estimate is used to determine the verification dose from the radiation dose tables specified in AAMI TIR 33.
- 3.3. The verification dose (sub-lethal) provides a SAL of 10^{-1} . A verification experiment must be performed to verify that the product bioburden resistance is less than or equal to the standard distribution of resistances used in the AAMI radiation guidelines.
- 3.4. Following completion of the study, a final report shall be generated by SteriPro, which shall be signed and approved by designated individuals from SteriPro, and Kimberly-Clark. This report shall be submitted to Kimberly-Clark and SteriPro will retain a copy as specified in the SteriPro procedure for record retention.

4. Terms and Definitions

Refer to ANSI/AAMI/ISO 11137:2006, AAMI TIR 33, and ANSI/AAMI/ISO 11737:2006 for definitions of terminology.

5. Responsibilities

5.1. Contract Irradiator

Sterigenics, Corona or Charlotte will be responsible for all equipment, process qualification, dosimeter calibration, and all documentation involving the ExCell irradiator's validation. A certificate of processing will be provided for the product in this study. All other Sterigenics records that are specific to this study will be available to the sponsor upon request or audit.

5.2. Contract Laboratory

SteriPro Labs, Itasca will perform the necessary microbiological testing for this validation and will provide all necessary documentation for the Final Report. DNV Certification, certificate numbers 2005-OSL-AQ-7662 and 2005-OSL-AQ-0212 certify SteriPro Labs to ISO 9001 and ISO 13485.

6. Product Specifications

6.1. Product Sample Amounts

Forty-eight (48) finished, routine product samples will be submitted in standard, final packaging format for all testing. These units shall be pulled after all steps of production except sterilization and be produced under current good manufacturing practice conditions. From the 48 product samples, there shall be three independent lots of ten samples each for bioburden determination. The 18 remaining samples may come from one or more production lots.



6.2. Sample Item Portion (SIP)

The SIP used for all testing will be 0.10. The SIP that will be tested as the test sample will consist of different parts of the coverall for a total SIP of 0.10.

6.3. Sample Preparation

Additional sample prep is needed prior to sterilization in order to facilitate testing.

7. Bioburden Study Method

7.1. Recovery Determination

7.1.1. Efficiency of Recovery Factor (ERF) will be determined using a specific bioburden recovery test procedure, which will be performed on a minimum of five samples taken from one or more production lots. This test is performed to determine the percentage of microorganisms that can be recovered from a product.

7.1.2. Averaging the recovery obtained from the samples tested will derive the recovery factor. The bioburden test results for each lot will be adjusted by applying the ERF, in order to obtain a theoretical bioburden estimate. This theoretical bioburden estimate is a more accurate representation of the actual number of microorganisms on the product.

7.2. Recovery Test Method

The bioburden recovery test method for the product will be performed using the repetitive extraction method or inoculated recovery method. The extraction method will be the same as the method used for the bioburden determination. This testing will be conducted using test parameters outlined in ANSI/AAMI/ISO 11737-1.

7.3. Bioburden Determination

Ten samples each from three independent lots will be tested for bioburden using a specific test procedure. Each lot will have the results reported in colony forming units (CFU), with the ERF applied. The bioburden test will include aerobic bacteria and fungal enumerations.

7.4. Bioburden Test Method

The bioburden test method will be performed by immersion of the SIP. This testing will be conducted using test parameters defined in ANSI/AAMI/ISO 11737-1.

8. Verification Study Method

8.1. Verification Dose Determination

8.1.1. A verification dose will be determined using the tables specified in AAMI TIR 33. The verification dose determination will be based on the final bioburden estimate for the product.

8.1.2. Thirteen packaged verification samples will be sent to Sterigenics for irradiation at the calculated verification dose. The actual dose delivered will be measured and documented by Sterigenics. Sterigenics will send the samples directly to the contract laboratory after the verification dose has been performed.



8.2. Verification Dose Range

If the maximum delivered dose exceeds the verification dose by more than 10%, the verification dose shall be repeated. If the maximum and minimum delivered dose is less than 90% of the verification dose, the verification dose may be repeated. If the delivered dose is less than 90% of the verification dose, and on the tests of sterility acceptable results are obtained, the verification experiment need not be repeated.

8.3. Test of Sterility

The test of sterility requires ten of the verification dose samples. The results will be reported as number of samples with growth and/or the number of samples with negative growth for the ten verification dose samples.

8.4. Test of Sterility Method

The test method will be performed by direct immersion. The test will be conducted using test parameters outlined in AAMI TIR 33 and ANSI/AAMI/ISO 11737-2.

8.5. Bacteriostasis/Fungistasis Determination

The bacteriostasis/fungistasis test requires three of the verification dose samples. This test is a validation of the test of sterility. This test will be conducted to verify that no bacteriostatic and fungistatic activity, which might compromise the sensitivity of the sterility test method, was exhibited by the samples, or formed by the verification dose exposure. The test results will be reported as a pass or fail.

8.6. Bacteriostasis/Fungistasis Test Method

The testing method will be the same as the method used for the test of sterility. The test will be performed using parameters outlined in the current USP.

9. Acceptance Criteria

Interpretation of results will be acceptable or unacceptable, as defined in AAMI TIR 33.

9.1. Verification is accepted if there are no more than one positive sterility test units out of the ten tested.

9.2. If two positives occur, perform another sterility test on ten additional units that have been irradiated at the same verification dose determined above. Upon completion of the second sterility test, add the number of positives from the two tests together. If the total number is two positives, verification is accepted.

9.3. If three or more positives occur, verification is not accepted. If the positive sterility units cannot be attributed to incorrect testing or dosing, an alternative dose determination method should be used unless the cause of the failure can be identified and corrected.

9.4. Bacteriostasis/Fungistasis test passes.



SteriPro.
Consulting
A Division of
Sterigenics International, Inc.

VD-Max32.5 Radiation Validation
Kimberly-Clark

Issued April 12, 2010
Protocol # 797100277-P Rev.0
Page 8 of 8

10. Routine Sterilization

- 10.1. The routine sterilization dose is based on the acceptable results as outlined in Section 9 of this protocol. The 32.5-kGy minimum sterilization dose is considered valid for achieving a 10^{-6} SAL for the product listed.
- 10.2. With completion and acceptance of this validation study, subsequent batches of the product may be sterilized at a minimum dose of 32.5-kGy and released for use based only on the dosimeters indicating that the minimum SAL of 10^{-6} dose has been delivered to the product.
- 10.3. Dose audits must be performed according to an established schedule, as indicated in ANSI/AAMI/ISO 11137-1.

11. References

- 11.1. ANSI/AAMI/ISO 11737-1:2006, Sterilization of health care products – Microbiological methods – Part 1: Determination of the population of microorganisms on product
- 11.2. ANSI/AAMI/ISO 11737-2:2009, Sterilization of medical devices – Microbiological methods – Part 2: Tests of sterility performed in the definition, validation and maintenance of a sterilization process
- 11.3. ANSI/AAMI/ISO 11137-1:2006, Sterilization of health care products – Radiation – Part 1: Requirements for development, validation, and routine control of a sterilization process for medical devices
- 11.4. ANSI/AAMI/ISO 11137-2:2006, Sterilization of health care products – Radiation – Part 2: Establishing the sterilization dose
- 11.5. AAMI TIR 33:2005, Sterilization of health care products – Radiation – Substantiation of a selected sterilization dose – Method VD-Max
- 11.6. USP/NF, U.S. Pharmacopoeia (current version)



BIOBURDEN TEST REPORT

Procedure Reference: LB-MIC-004

SteriPro® Labs WO#: 401711-MIC-004-I

Page 1 of 1

Date Received: 03/29/10

Customer: Kimberly-Clark 1400 Holcomb Bridge Road Roswell, GA 30076	Product: KIMTECH PURE* A5 Cleanroom Sterile Apparel- Boots 2XL Cat / Part #: 12920 Lot #: AR007702X
--	---

Customer Specification Sheet# / Rev #: I-004-411/ Rev. 2 Efficiency Recovery Factor (ERF): N/A

<u>Test Media</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. Date</u>
Tryptic Soy Agar (TSA):	Biomerieux	ITMFR432	07/14/10
Sabouraud Dextrose Agar (SDA):	SteriPro	IT01703132	03/17/11
Phosphate Buffered Saline (PBS):	SteriPro	IT02303143	03/23/11

Sample Preparation: Each sample was immersed.

Total Rinse Volume: 200mL Volume Extracted per Organism Type: 40mL

Enumeration Method: Pour Plate X Filtration Surface

TSA Incubation Temperature: 30-35°C SDA Incubation Temperature: 20-25°C

Date Extracted/Incubated: 03/30/10 Date TSA Enumerated: 04/02/10 Date SDA Enumerated: 04/05/10

TEST RESULTS (Colony Forming Units (CFU) per Device):

Sample ID	Aerobes (TSA)	Fungi-Yeast/Mold (SDA)
1	120	<5
2	120	<5
3	130	<5
4	115	<5
5	135	10
6	235	5
7	150	10
8	135	5
9	175	5
10	125	<5
Total Average Bioburden/Device (calculated with ERF, if applicable)	144.0	6.0

Control Results: TSA 0 SDA 0 PBS 0

Comments:

Prepared By: Alex Castro Date: 4/7/10

Reviewed By: Brian Moran Date: 4/7/10

The test results relate only to the samples as provided and tested. This report may not be reproduced, except in full, without written approval from SteriPro Labs.

SteriPro Labs expressly states that it makes no representation or warranty regarding the adequacy of the samples submitted for testing for any specific use or application, that being the determined responsibility of the sponsoring client. SteriPro Labs' liability for any loss or damage resulting from its actions or failure to act shall not exceed the cost of the testing performed, and SteriPro Labs shall not be liable for any incidental or consequential damages.



BIOBURDEN TEST REPORT

Procedure Reference: LB-MIC-004

SteriPro® Labs WO#: 401710-MIC-004-I

Page 1 of 1

Date Received: 03/29/10

Customer: Kimberly-Clark 1400 Holcomb Bridge Road Roswell, GA 30076	Product: KIMTECH PURE* A5 Cleanroom Sterile Apparel- Hood
	Cat / Part #: 88807
	Lot #: AR007502X

Customer Specification Sheet# / Rev #: I-004-411/ Rev. 2 Efficiency Recovery Factor (ERF): N/A

<u>Test Media</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. Date</u>
Tryptic Soy Agar (TSA):	Biomerieux	ITMFR432	07/14/10
Sabouraud Dextrose Agar (SDA):	SteriPro	IT01703132	03/17/11
Phosphate Buffered Saline (PBS):	SteriPro	IT02303143	03/23/11

Sample Preparation: Each sample was immersed.

Total Rinse Volume: 200mL Volume Extracted per Organism Type: 40mL

Enumeration Method: Pour Plate X Filtration Surface

TSA Incubation Temperature: 30-35°C SDA Incubation Temperature: 20-25°C

Date	Date TSA	Date SDA
Extracted/Incubated: <u>03/30/10</u>	Enumerated: <u>04/02/10</u>	Enumerated: <u>04/05/10</u>

TEST RESULTS (Colony Forming Units (CFU) per Device):

Sample ID	Aerobes (TSA)	Fungi-Yeast/Mold (SDA)
1	175	<5
2	210	30
3	200	5
4	180	5
5	175	5
6	200	<5
7	215	10
8	190	5
9	270	15
10	125	10
Total Average Bioburden/Device (calculated with ERF, if applicable)	194.0	9.5

Control Results: TSA 0 SDA 0 PBS 0

Comments:

Prepared By: Alex Castro Date: 4/7/10

Reviewed By: [Signature] Date: 4/7/10

The test results relate only to the samples as provided and tested. This report may not be reproduced, except in full, without written approval from SteriPro Labs.

SteriPro Labs expressly states that it makes no representation or warranty regarding the adequacy of the samples submitted for testing for any specific use or application, that being the determined responsibility of the sponsoring client. SteriPro Labs' liability for any loss or damage resulting from its actions or failure to act shall not exceed the cost of the testing performed, and SteriPro Labs shall not be liable for any incidental or consequential damages.



BIOBURDEN EXHAUSTIVE RECOVERY VALIDATION TEST REPORT

Procedure Reference: LB-MIC-004

SteriPro® Labs WO#: 401712-MIC-004-1

Page 1 of 2

Date Received: 03/29/10

Customer:	Kimberly-Clark 1400 Holcomb Bridge Road Roswell, GA 30076	Product:	KIMTECH PURE*A5 Cleanroom Sterile Apparel-coveralls-6XL
		Cat / Part #:	12914
		Lot #:	AR007602A

Customer Specification Sheet# / Rev #: I-004-411/ Rev. 2 Efficiency Recovery Factor (ERF): N/A

<u>Test Media</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. Date</u>
Tryptic Soy Agar (TSA):	Biomerieux	ITMFR437	07/29/10
Sabouraud Dextrose Agar (SDA):	SteriPro	IT01703132	03/17/11
Phosphate Buffered Saline (PBS):	SteriPro	IT02303143	03/23/11

Sample Preparation: For each sample, an SIP of 10% was cut and immersed in PBS

Total Rinse Volume: 200mL Volume Extracted per Organism Type: 40mL

Enumeration Method: Pour Plate X Filtration Surface

TSA incubation Temperature: 30-35°C SDA Incubation Temperature: 20-25°C

Date	Date TSA	Date SDA
Extracted/Incubated: <u>04/01/10</u>	Enumerated: <u>04/05/10</u>	Enumerated: <u>04/06/10</u>

See Following Page(s) for Repetitive Wash Results

Calculated Efficiency Recovery Factor (ERF): 0.27

Comments:

Prepared By: *Alvaro Castro* Date: 4/6/10

Reviewed By: *Brian Watson* Date: 4/6/10

The test results relate only to the samples as provided and tested. This report may not be reproduced, except in full, without written approval from SteriPro Labs.

SteriPro Labs expressly states that it makes no representation or warranty regarding the adequacy of the samples submitted for testing for any specific use or application, that being the determined responsibility of the sponsoring client. SteriPro Labs' liability for any loss or damage resulting from its actions or failure to act shall not exceed the cost of the testing performed, and SteriPro Labs shall not be liable for any incidental or consequential damages.



BIOBURDEN EXHAUSTIVE RECOVERY VALIDATION TEST REPORT

Procedure Reference: LB-MIC-004

SteriPro® Labs WO#: 401712-MIC-004-I

Page 2 of 2

TEST RESULTS (Colony Forming Units (CFU) per Device):

FIRST WASH

Sample ID	Aerobes (TSA)	Fungi-Yeast/Mold (SDA)
1	1850	50
2	2200	150
3	1050	50
4	1850	<50
5	1200	50
Total Average Bioburden/Device	1630	70

SECOND WASH

Sample ID	Aerobes (TSA)	Fungi-Yeast/Mold (SDA)
1	2300	50
2	1800	50
3	2850	50
4	2650	<50
5	1750	<50
Total Average Bioburden/Device	2270	50

THIRD WASH

Sample ID	Aerobes (TSA)	Fungi-Yeast/Mold (SDA)
1	2900	50
2	2150	100
3	2000	100
4	2550	50
5	1700	50
Total Average Bioburden/Device	2300	70

Control Results: TSA 0 SDA 0 PBS 0

The test results relate only to the samples as provided and tested. This report may not be reproduced, except in full, without written approval from SteriPro Labs.

SteriPro Labs expressly states that it makes no representation or warranty regarding the adequacy of the samples submitted for testing for any specific use or application, that being the determined responsibility of the sponsoring client. SteriPro Labs' liability for any loss or damage resulting from its actions or failure to act shall not exceed the cost of the testing performed, and SteriPro Labs shall not be liable for any incidental or consequential damages.



BIOBURDEN TEST REPORT

Procedure Reference: LB-MIC-004

SteriPro® Labs WO#: 401709-MIC-004-I

Page 1 of 1

Date Received: 03/29/10

Customer: Kimberly-Clark 1400 Holcomb Bridge Road Roswell, GA 30076	Product: KIMTECH PURE* A5 Cleanroom Sterile Apparel- Coveralls-6XL
	Cat / Part #: 12914
	Lot #: AR007602A

Customer Specification Sheet# / Rev #: I-004-411/ Rev. 2 Efficiency Recovery Factor (ERF): 0.27

<u>Test Media</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. Date</u>
Tryptic Soy Agar (TSA):	Biomerieux	ITMFR432	07/14/10
Sabouraud Dextrose Agar (SDA):	SteriPro	IT01703132	03/17/11
Phosphate Buffered Saline (PBS):	SteriPro	IT02303143	03/23/11

Sample Preparation: An SIP of 10% of sample was cut and immersed.

Total Rinse Volume: 200mL Volume Extracted per Organism Type: 40mL

Enumeration Method: Pour Plate X Filtration Surface

TSA Incubation Temperature: 30-35°C SDA Incubation Temperature: 20-25°C

Date Extracted/Incubated: 03/30/10 Date TSA Enumerated: 04/02/10 Date SDA Enumerated: 04/05/10

TEST RESULTS (Colony Forming Units (CFU) per Device):

Sample ID	Aerobes (TSA)	Fungi-Yeast/Mold (SDA)
1	1750	<50
2	1800	200
3	1850	50
4	3050	50
5	2250	150
6	1700	200
7	2950	100
8	2000	150
9	2750	200
10	1950	200
Total Average Bioburden/Device (calculated with ERF, if applicable)	8166.7	500.0

Control Results: TSA 0 SDA 0 PBS 0

Comments:

Prepared By: Alex Castro Date: 4/4/10

Reviewed By: Brian Mason Date: 4/7/10

The test results relate only to the samples as provided and tested. This report may not be reproduced, except in full, without written approval from SteriPro Labs.

SteriPro Labs expressly states that it makes no representation or warranty regarding the adequacy of the samples submitted for testing for any specific use or application, that being the determined responsibility of the sponsoring client. SteriPro Labs' liability for any loss or damage resulting from its actions or failure to act shall not exceed the cost of the testing performed, and SteriPro Labs shall not be liable for any incidental or consequential damages.



BIOBURDEN TEST REPORT

Procedure Reference: LB-MIC-004

SteriPro® Labs WO#: 407027-MIC-004-I

Page 1 of 1

Date Received: 04/07/10

Customer: Kimberly-Clark 1400 Holcomb Bridge Road Roswell, GA 30076	Product: KIMTECH PURE* A5 Cleanroom Sterile Apparel-Coveralls-6XL
	Cat / Part #: 12914
	Lot #: AR010402B

Customer Specification Sheet# / Rev #: I-004-411/ Rev. 3 Efficiency Recovery Factor (ERF): 0.27

<u>Test Media</u>	<u>Manufacturer</u>	<u>Lot No.</u>	<u>Exp. Date</u>
Tryptic Soy Agar (TSA):	Biomerieux	ITMFR437	07/29/10
Sabouraud Dextrose Agar (SDA):	SteriPro	IT01703132	03/17/11
Phosphate Buffered Saline (PBS):	SteriPro	IT00104165	04/01/11

Sample Preparation: Each SIP of 10% was cut and immersed in PBS.

Total Rinse Volume: 200mL Volume Extracted per Organism Type: 40mL

Enumeration Method: Pour Plate X Filtration Surface

TSA Incubation Temperature: 30-35°C SDA Incubation Temperature: 20-25°C

Date	Date TSA	Date SDA
Extracted/Incubated: <u>04/08/10</u>	Enumerated: <u>04/12/10</u>	Enumerated: <u>04/13/10</u>

TEST RESULTS (Colony Forming Units (CFU) per Device):

Sample ID	Aerobes (TSA)	Fungi-Yeast/Mold (SDA)
1	2300	150
2	3200	200
3	2350	100
4	2850	<50
5	5250	<50
6	4500	100
7	3400	50
8	2000	<50
9	3250	50
10	1850	50
Total Average Bioburden/Device (calculated with ERF, if applicable)	11463.0	314.8

Control Results: TSA 0 SDA 0 PBS 0

Comments:

Prepared By: Alex Castro Date: 4/14/10

Reviewed By: Bright Watson Date: 4/14/10

The test results relate only to the samples as provided and tested. This report may not be reproduced, except in full, without written approval from SteriPro Labs.

SteriPro Labs expressly states that it makes no representation or warranty regarding the adequacy of the samples submitted for testing for any specific use or application, that being the determined responsibility of the sponsoring client. SteriPro Labs' liability for any loss or damage resulting from its actions or failure to act shall not exceed the cost of the testing performed, and SteriPro Labs shall not be liable for any incidental or consequential damages.



BIOBURDEN TEST REPORT

Procedure Reference: LB-MIC-004

SteriPro® Labs WO#: 407026-MIC-004-I

Page 1 of 1

Date Received: 04/07/10

Customer: Kimberly-Clark 1400 Holcomb Bridge Road Roswell, GA 30076	Product: KIMTECH PURE* A5 Cleanroom Sterile Apparel-Coveralls-6XL
Cat / Part #: 12914	Lot #: AR010402C

Customer Specification Sheet# / Rev #: I-004-411/ Rev. 3 Efficiency Recovery Factor (ERF): 0.27

Test Media	Manufacturer	Lot No.	Exp. Date
Tryptic Soy Agar (TSA):	Biomerieux	ITMFR437	07/29/10
Sabouraud Dextrose Agar (SDA):	SteriPro	IT01703132	03/17/11
Phosphate Buffered Saline (PBS):	SteriPro	IT00104165	04/01/11

Sample Preparation: Each SIP of 10% was cut and immersed in PBS.

Total Rinse Volume: 200mL Volume Extracted per Organism Type: 40mL

Enumeration Method: Pour Plate X Filtration Surface

TSA Incubation Temperature: 30-35°C SDA Incubation Temperature: 20-25°C

Date	Date TSA	Date SDA
Extracted/Incubated: <u>04/08/10</u>	Enumerated: <u>04/12/10</u>	Enumerated: <u>04/13/10</u>

TEST RESULTS (Colony Forming Units (CFU) per Device):

Sample ID	Aerobes (TSA)	Fungi-Yeast/Mold (SDA)
1	4250	<50
2	4800	100
3	2050	<50
4	2150	100
5	3900	150
6	3100	150
7	1800	<50
8	2250	50
9	2700	50
10	2750	100
Total Average Bioburden/Device (calculated with ERF, if applicable)	11018.5	314.8

Control Results: TSA 0 SDA 0 PBS 0

Comments:

Prepared By: Alex Castro Date: 4/14/10

Reviewed By: Bryan Miller Date: 4/14/10

The test results relate only to the samples as provided and tested. This report may not be reproduced, except in full, without written approval from SteriPro Labs.

SteriPro Labs expressly states that it makes no representation or warranty regarding the adequacy of the samples submitted for testing for any specific use or application, that being the determined responsibility of the sponsoring client. SteriPro Labs' liability for any loss or damage resulting from its actions or failure to act shall not exceed the cost of the testing performed, and SteriPro Labs shall not be liable for any incidental or consequential damages.



Dose Calculation for Kimberly-Clark KIMTECH PURE*A5 Cleanroom Sterile Apparel

Based on the Total Recoverable Aerobic and Fungi Bioburden results from three independent lots of the KIMTECH PURE* A5 Cleanroom Sterile Apparel, the theoretical overall average taken from the three lots was selected to calculate the subprocess Verification dose. The Recovery Factor was determined to be 0.27.

Per AAMI TIR33: Method VD-Max30 guidelines, the Sub-process Verification dose is based on the overall average bioburden from three lots, unless one of the averages is two or more times greater than that of that overall average. The verification dose was derived from the theoretical bioburden average of the three lots. The theoretical lot averages are as follows:

<u>Lot Number</u>	<u>Total Bioburden (Aerobic and Fungal) As colony forming units (cfu) per device</u>
AR007602A	8666.7 cfu/device
AR010402B	11777.8 cfu/device
AR010402C	11333.3 cfu/device

The overall average bioburden for the three lots, including the recovery factor, is 10592.6 cfu per device. Based on 10592.6 cfu per device, and utilizing the SIP verification dose calculation, the verification dose was determined directly from Table A.7 of the AAMI TIR33 guidance. The verification dose for the device is **9.9 kGy**.

In accordance with the AAMI TIR33: Method VD-Max30 guidelines, ten units of product should be sampled from a single production lot and irradiated at the verification dose of 9.9 kGy \pm 10%. After irradiation the samples will be sent to SteriPro Labs to be placed on test of sterility.

If these ten units, which will have been irradiated at 9.9 kGy, meet the criteria set forth in the AAMI TIR33: Method VD-Max30 guidelines (no more than one positive per ten units), then the minimum sterilization dose from a sterility assurance level would be 30.0 kGy.

Best regards,

Zabrina Tumaitis
Consultant, SteriPro Consulting



Certificate of Processing

STERIGENICS 344 Bonnie Circle Corona CA 92880
 TEL 951 340-0700 FAX www.sterigenics.com

R55480102
 RIS0003

04/19/10 16:05:51 GMT
 Page - 1 of 1

Customer Name: SteriPro Consulting
 P.O.# 12334270 / KIMBERLY CLARK

Processing Facility: Corona

Work Order # 412952
 Sales Order # 363808

X_STERIPRO_18

Irradiation Date/Time: 04/18/10 17:03:00 GMT
 Irradiation Cell: EXCELL

SO Line #	Qty	UOM	Customer Item Number / Customer Item Description	Customer Lot Number / Customer Load Number
101.00	1	CA	X_CARTON_STERIPRO_18	AR007602B COVERALLS - 6XL
	1	CA	Total	

Quality Test Summary

-----Signed By-----

Op#	Quality Test Description	Result	Pass/Fail	User	Date / Time
450.00	Minimum Dose	9.4 kGy	Pass	JGARCIA Jose Garcia Reason Code Test	04/19/10 01:38:28 GMT
450.00	Maximum Dose	10.2 kGy	Pass	JGARCIA Jose Garcia Reason Code Test	04/19/10 01:38:44 GMT

Sterigenics certifies that the materials listed above (as described by the Manufacturer) received the indicated doses within the precision and accuracy of the dosimetry system employed.

Electronically Signed By: Annette Posada
 Work Order Completions

Date: 04/19/10 16:00:47 GMT



STERILITY VALIDATION (B&F) TEST REPORT

Procedure Reference: LB-MIC-027

SteriPro® Labs WO#: 415045-MIC-027-I

Page 1 of 1

Date Received: 04/20/10

Date On-Test: 04/21/10

Date Off-Test: 04/26/10

Customer: Kimberly Clark 1400 Holcomb Bridge Road Roswell, GA 30076	Product: KIMTECH PURE* A5 Cleanroom Sterile Apparel- Coveralls -6XL 12914 Cat / Part #: Lot #: AR007602B Load #: N/A Sterilization Run: 412952 Date Sterilized: 04/19/10
--	---

<u>Test Media</u>	<u>Manufacturer</u>	<u>Volume</u>	<u>Lot No.</u>	<u>Exp. Date</u>
TSB	SteriPro	3000mL	IT01204185 IT01904195	04/12/11 04/19/11

Product Sterility Customer Specification Sheet# / Revision: I-036-797/Rev. 0

Test Method:
Immersion of SIP

Test Results: X PASS FAIL

ORGANISM	TSB	
	Control	Sample
<i>Bacillus subtilis</i> (ATCC #6633)	+	+
<i>Candida albicans</i> (ATCC #10231)	+	+
<i>Aspergillus niger</i> (ATCC #16404)	+	+

Comments:
N/A

Prepared By: Date: 4/27/10

Reviewed By: Date: 4/27/10

The test results relate only to the samples as provided and tested. This report may not be reproduced, except in full, without written approval from SteriPro Labs. SteriPro Labs expressly states that it makes no representation or warranty regarding the adequacy of the samples submitted for testing for any specific use or application, that being the determined responsibility of the sponsoring client. SteriPro Labs' liability for any loss or damage resulting from its actions or failure to act shall not exceed the cost of the testing performed, and SteriPro Labs shall not be liable for any incidental or consequential damages.



PRODUCT STERILITY TEST REPORT

Procedure Reference: LB-MIC-036

SteriPro® Labs WO#: 415039-MIC-036-I

Page 1 of 1

Date Received: 04/20/10

Date On-Test: 04/21/10

Date Off-Test: 05/05/10

Customer: Kimberly –Clark 1400 Holcomb Bridge Road Roswell, GA 30076	Product: KIMTECH PURE* A5 Cleanroom Sterile Appareal-Coveralls-6XL
Cat / Part #: 12914	Lot #: AR007602B
Load #: AR007602B	Sterilization Run: 412952
Date Sterilized: 04/19/10	

<u>Test Media</u>	<u>Manufacturer</u>	<u>Volume</u>	<u>Lot No.</u>	<u>Exp. Date</u>
Tryptic Soy Broth (TSB)	SteriPro Labs	3000mL	IT01204185	04/12/11

Number of Samples: 10

Customer Specification Sheet# / Revision #: I-036-797/ Rev. 0

Test Method:

Immersion of SIP.

Test Results:

TSB:	<u> X </u>	No Growth	<u> </u>	Growth
Open Control:	<u> X </u>	No Growth	<u> </u>	Growth

Results Meet Criteria: X YES NO

Attachments Included: N/A

Comments: N/A

Prepared By: Alex Claster Date: 5/5/10

Reviewed By: Catherin Beat Date: 5/6/10

The test results relate only to the samples as provided and tested. This report may not be reproduced, except in full, without written approval from SteriPro Labs. SteriPro Labs expressly states that it makes no representation or warranty regarding the adequacy of the samples submitted for testing for any specific use or application, that being the determined responsibility of the sponsoring client. SteriPro Labs' liability for any loss or damage resulting from its actions or failure to act shall not exceed the cost of the testing performed, and SteriPro Labs shall not be liable for any incidental or consequential damages.

Dose setting Report

Kimberly-Clark Corporation

1400 Holcomb Bridge Road, Roswell, Georgia

The following sample(s) was/were submitted and identified on behalf of the applicant as:

Kimtech Pure A5 Sterile Integrated Hood and Mask

Date of Sample Receipt 2013/03/04

Lab Test ID 13-033A

Date on Test 2013/03/04

Test Item Dose Setting

Test Method ISO 11137-2-2012: Method 1

Signature

Tudy Zhu 2013-04-01
 Edited by Date

Luke Song 2013-04-01
 Reviewed by Date

Seagle Xu 2013-04-01
 Approved by Date

Shirley McCoy 2013-04-01
 Kimberly-Clark Professional

Revision

0	2013/04/01	First edition
Revision No.	Date	Revision Description

• **Tested sample description**

Sample information	
Sample name	Kimtech Pure A5 Sterile Integrated Hood and Mask
Product code	36072
Lot [#]	First batch, second batch, third batch
Number of Sample	138 samples
SIP	1.0

• **Sample photo**



• **Test results**

✦ **Bioburden validation (Inoculation)**

Bioburden validation test results(Sample Lot: Second batch)					
Sample ID	Counted	PF	Recovered per sample(CFU)	Confirmed Inoculation level(CFU)	ERF
1	14	2.0	28	52/48	0.56
2	13		26		0.52
3	14		28		0.56
4	13		26		0.52
5	10		20		0.40
Average	12.8	NA	25.6	50	0.51
C.F (Correction Factor)		2.0			

✧ Bioburden test

Bioburden Test Result (Sample Lot: First batch)						
ID	CFU count		CFU Counted	P.F	C.F	CFU/ SIP sample
	Aerobes	Fungi				
1	164	87	251	4	2.0	2008
2	135	22	157			1256
3	221	87	308			2464
4	156	112	268			2144
5	142	47	189			1512
6	348	80	428			3424
7	98	45	143			1144
8	125	8	133			1064
9	147	48	195			1560
10	127	64	191			1528
control	0	0	N/A	N/A	N/A	N/A
SIP Average	1810.4 CFU/SIP sample					
Batch 1 Average	1810.4 CFU/Device					
Bioburden Test Result (Sample Lot: Second batch)						
ID	CFU count		CFU Counted	P.F	C.F	CFU/ SIP sample
	Aerobes	Fungi				
1	259	67	326	4	2.0	2608
2	91	40	131			1048
3	301	68	369			2952
4	424	42	466			3728
5	147	52	199			1592
6	324	124	448			3584
7	235	68	303			2424
8	184	10	194			1552

9	242	62	304			2432
10	187	74	261			2088
control	0	0	N/A	N/A	N/A	N/A
SIP Average	2400.8 CFU/SIP sample					
Batch 2 Average	2400.8 CFU/Device					
Bioburden Test Result (Sample Lot: Third batch)						
ID	CFU count		CFU Counted	P.F	C.F	CFU/ SIP sample
	Aerobes	Fungi				
1	145	56	201	4	2.0	1608
2	149	10	159			1272
3	260	56	316			2528
4	145	48	193			1544
5	140	34	174			1392
6	256	52	308			2464
7	88	79	167			1336
8	98	25	123			984
9	231	60	291			2328
10	296	84	380			3040
control	0	0	N/A	N/A	N/A	N/A
SIP Average	1849.6 CFU/SIP sample					
Batch 3 Average	1849.6 CFU/Device					

✧ **Establishing sterilization dose**

Establishing sterilization dose			
Overall average bioburden(SIP)	Verification dose (SIP sample)	Overall average bioburden (Device)	Sterilization dose (10^{-6})
2020.3 CFU	12.0 kGy	2020.3 CFU	26.1 kGy

Note: Overall average bioburden= (batch1+batch2+batch3)/3= (1810.4+2400.8+1849.6)/3= 2020.3 CFU/device

✧ **Irradiation of verification dose**

Verification dose is irradiated on 100 samples (Lot: XN306301X) within the $\pm 10\%$ of target dose 12.0 kGy. Detail information refers to **Certificate of Irradiation for Test Sample** from **Sterigenics Shanghai E-Beam Co., Ltd (PO20130314128391)**.

✧ **Sterility test validation (Bacteriostasis & Fungistasis Test)**

Sterility Test Validation (B/F) Result			
Culture	<i>Bacillus subtilis</i> ATCC 6633	<i>Candida albicans</i> ATCC10231	<i>Aspergillus brasiliensis</i> ATCC16404
Test Sample	Positive	Positive	Positive
Inoculated Control	Positive	Positive	Positive
Inoculum Level(CFU)	31	39	30
Conclusion	The products of Kimtech Pure A5 Sterile Integrated Hood and Mask (Code: 36072) do not exist bacteriostatic and fungistatic properties, or such properties have been eliminated through the test.		

✧ **Sterility test**

Sterility Test Result	
SIP	1.0
Sample number	100
Type of Media	TSB
Media Volume	800mL
Incubation Period	14 days
Incubation Temperature	28°C - 32°C
Results	1 Positive

• **Conclusion**

From validation results show, the product of **Kimtech Pure A5 Sterile Integrated Hood and Mask (Code: 36072)** **PASS** the dose setting by using Method 1 according to ISO 11137-2. A sterility assurance level (SAL) of 10^{-6} is confirmed when irradiating the product by a sterilization dose of 26.1 kGy for routine production.

• **References**

- ✧ ISO 11737-1:2006 Sterilization of health care products - Microbiological methods - Part 1: Determination of the population of microorganisms on product
- ✧ ISO 11737-2:2009 Sterilization of medical devices---Microbiological methods---Part2: Tests of sterility performed in the definition, validation and maintenance of a sterilization process

- ◇ ISO 11137-2:2006 Sterilization of health care products---Radiation---Part 2: Establishing the sterilization dose
- ◇ Sterigenics internal Work Instruction SHEB-WI-LB-MIC-003
- ◇ Sterigenics internal Work Instruction SHEB-WI-LB-MIC-016

- **Remarks**

- ◇ The test report is invalid unless signed by editor, reviewer and approver.
- ◇ The test report is invalid if altered.
- ◇ Please contact testing laboratory within 15 days after receiving the test report if any objection to the report, otherwise it will not be accepted.
- ◇ The test report is only responsible for the sample provided by customer.
- ◇ The test report cannot be used for any commercial purpose unless approved by testing laboratory.
- ◇ Tested by SteriPro laboratory, Sterigenics Shanghai E-Beam Ltd.
No.588 ChuanTu Road, Chuansha. Pudong, Shanghai, China. 201202.
Tel(86-21) 58594680 Fax(86-21)58599310

=====End of report=====

Dose setting Report

Kimberly-Clark Corporation

1400 Holcomb Bridge Road, Roswell, Georgia

The following sample(s) was/were submitted and identified on behalf of the applicant as:

Kimtech Pure A5 Sterile Sleeves

Date of Sample Receipt	2013/03/04
Lab Test ID	13-033A
Date on Test	2013/03/04
Test Item	Dose Setting
Test Method	ISO 11137-2-2012: Method 1

Signature

Tudy Zhu 2013-04-01
 Edited by Date

Luke Song 2013-04-01
 Reviewed by Date

Seagle Xu 2013-04-01
 Approved by Date

Jhurna McCoy 2013-04-01
 Kimberly-Clark Professional


Revision

0	2013/04/01	First edition
Revision No.	Date	Revision Description

• **Tested sample description**

Sample information	
Sample name	Kimtech Pure A5 Sterile Sleeves
Product code	36077
Lot#	First batch, second batch, third batch
Number of Sample	138samples
SIP	1.0

• **Sample photo**

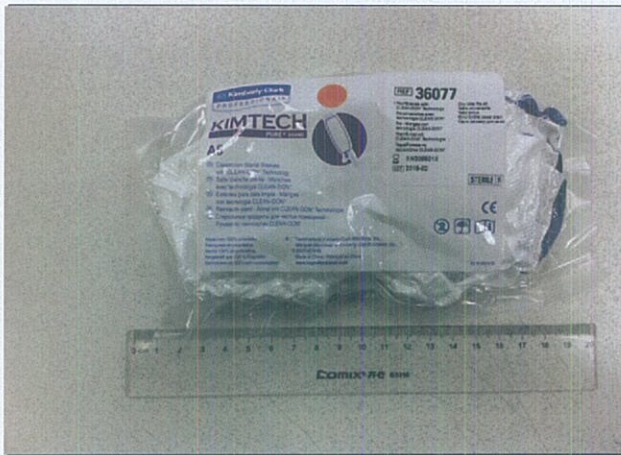

• **Test results**

◇ **Bioburden validation (Inoculation)**

Bioburden validation test results(Sample Lot: First batch)					
Sample ID	Counted	PF	Recovered per sample(CFU)	Confirmed Inoculation level(CFU)	ERF
1	22	1.5	33.0	52/48	0.66
2	18		27.0		0.54
3	25		37.5		0.75
4	16		24.0		0.48
5	21		31.5		0.63
Average	20.4	NA	30.6	50	0.61
C.F (Correction Factor)		1.7			

✧ Bioburden test

Bioburden Test Result (Sample Lot: First batch)						
ID	CFU count		CFU Counted	P.F	C.F	CFU/ SIP sample
	Aerobes	Fungi				
1	1620	147	1767	3	1.7	9011.7
2	2240	259	2499			12744.9
3	2410	84	2494			12719.4
4	2520	138	2658			13555.8
5	1780	187	1967			10031.7
6	740	124	864			4406.4
7	960	67	1027			5237.7
8	1780	252	2032			10363.2
9	2520	51	2571			13112.1
10	1460	54	1514			7721.4
control	0	0	N/A	N/A	N/A	N/A
SIP Average	9890.4 CFU/SIP sample					
Batch 1 Average	9890.4 CFU/Device					
Bioburden Test Result (Sample Lot: Second batch)						
ID	CFU count		CFU Counted	P.F	C.F	CFU/ SIP sample
	Aerobes	Fungi				
1	1180	50	1230	3	1.7	6273
2	117	26	143			729.3
3	222	47	269			1371.9
4	680	32	712			3631.2
5	146	55	201			1025.1
6	210	51	261			1331.1
7	226	56	282			1438.2
8	123	85	208			1060.8

9	112	38	150			765
10	292	82	374			1907.4
control	0	0	N/A	N/A	N/A	N/A
SIP Average	1953.3 CFU/SIP sample					
Batch 2 Average	1953.3 CFU/Device					
Bioburden Test Result (Sample Lot: Third batch)						
ID	CFU count		CFU Counted	P.F	C.F	CFU/ SIP sample
	Aerobes	Fungi				
1	1460	152	1612	3	1.7	8221.2
2	2100	39	2139			10908.9
3	1760	56	1816			9261.6
4	980	56	1036			5283.6
5	1540	82	1622			8272.2
6	420	21	441			2249.1
7	680	95	775			3952.5
8	1440	65	1505			7675.5
9	1980	34	2014			10271.4
10	1460	127	1587			8093.7
control	0	0	N/A	N/A	N/A	N/A
SIP Average	7419.0 CFU/SIP sample					
Batch 3 Average	7419.0 CFU/Device					

✦ **Establishing sterilization dose**

Establishing sterilization dose			
Overall average bioburden(SIP)	Verification dose (SIP sample)	Overall average bioburden (Device)	Sterilization dose (10^{-6})
6420.9 CFU	13.6 Gy	6420.9 CFU	27.9 KGy

Note: Overall average bioburden= (batch1+batch2+batch3)/3= (9890.4+1953.3+7419.0)/3= 6420.9 CFU/device

✦ **Irradiation of verification dose**

Verification dose is irradiated on 100 samples (Lot: XN306301X) within the $\pm 10\%$ of target dose 13.6 kGy. Detail information refers to **Certificate of Irradiation for Test Sample** from **Sterigenics Shanghai E-Beam Co., Ltd (PO20130313128358)**.

❖ **Sterility test validation (Bacteriostasis & Fungistasis Test)**

Sterility Test Validation (B/F) Result			
Culture	<i>Bacillus subtilis</i> ATCC 6633	<i>Candida albicans</i> ATCC10231	<i>Aspergillus brasiliensis</i> ATCC16404
Test Sample	Positive	Positive	Positive
Inoculated Control	Positive	Positive	Positive
Inoculum Level(CFU)	31	39	30
Conclusion	The products of Kimtech Pure A5 Sterile Sleeves (Code: 36077) do not exist bacteriostatic and fungistatic properties, or such properties have been eliminated through the test.		

❖ **Sterility test**

Sterility Test Result	
SIP	1.0
Sample number	100
Type of Media	TSB
Media Volume	400mL
Incubation Period	14 days
Incubation Temperature	28°C - 32°C
Results	2 Positive

• **Conclusion**

From validation results show, the product of **Kimtech Pure A5 Sterile Sleeves** (Code: **36077**) **PASS** the dose setting by using Method 1 according to ISO 11137-2. A sterility assurance level (SAL) of 10^{-6} is confirmed when irradiating the product by a sterilization dose of 27.9 kGy for routine production.

• **References**

- ❖ ISO 11737-1:2006 Sterilization of health care products - Microbiological methods - Part 1: Determination of the population of microorganisms on product
- ❖ ISO 11737-2:2009 Sterilization of medical devices---Microbiological methods---Part2: Tests of sterility performed in the definition, validation and maintenance of a sterilization process

- ◇ ISO 11137-2:2006 Sterilization of health care products---Radiation---Part 2: Establishing the sterilization dose
- ◇ Sterigenics internal Work Instruction SHEB-WI-LB-MIC-003
- ◇ Sterigenics internal Work Instruction SHEB-WI-LB-MIC-016

- **Remarks**

- ◇ The test report is invalid unless signed by editor, reviewer and approver.
- ◇ The test report is invalid if altered.
- ◇ Please contact testing laboratory within 15 days after receiving the test report if any objection to the report, otherwise it will not be accepted.
- ◇ The test report is only responsible for the sample provided by customer.
- ◇ The test report cannot be used for any commercial purpose unless approved by testing laboratory.
- ◇ Tested by SteriPro laboratory, Sterigenics Shanghai E-Beam Ltd.
No.588 ChuanTu Road, Chuansha. Pudong, Shanghai, China. 201202.
Tel(86-21) 58594680 Fax(86-21)58599310

=====End of report=====